



A Prospective, Randomized Investigation of a Novel Platinum Chromium Everolimus-Eluting Coronary Stent: The PLATINUM Trial

Gregg W. Stone MD
Columbia University Medical Center
The Cardiovascular Research Foundation

Disclosures



Scientific advisory boards for and honoraria
from Boston Scientific and Abbott Vascular, and
consultant to Medtronic

Background

- ◆ Advances in stent technology have continued to improve the clinical outcomes for patients undergoing PCI
- ◆ The cobalt chromium everolimus-eluting stent (**XIENCE V / PROMUS**) has established a new standard for clinical safety and efficacy, with numerous randomized trials demonstrating low rates of restenosis and stent thrombosis

Background

- ◆ A novel stent based on a new metal alloy has been developed, the platinum chromium EES (PtCr-EES; PROMUS Element), which uses the same durable, biocompatible, inert fluorocopolymer and antiproliferative agent as the predicate CoCr-EES, but with a modified scaffold designed for improved deliverability, vessel conformability, side-branch access, radiopacity, radial strength and fracture resistance



Everolimus-Eluting Stents




Everolimus concentration: 100 ug/cm²

Polymer: PBMA & PVDF-HFP (7μm thickness)

XIENCE V / PROMUS (CoCr-EES)

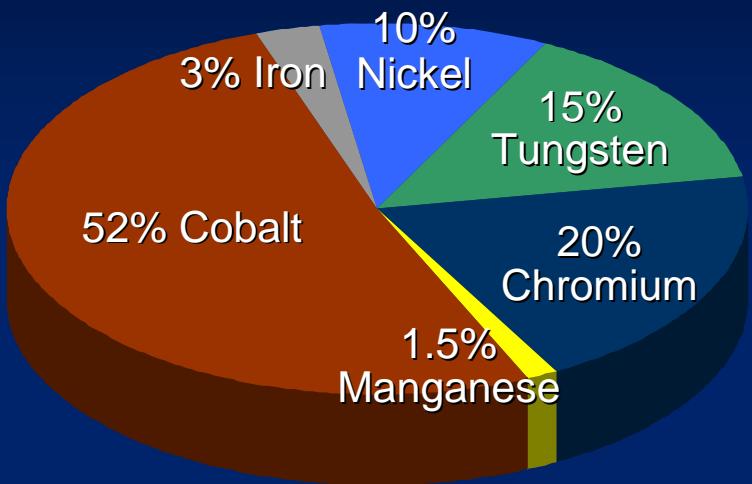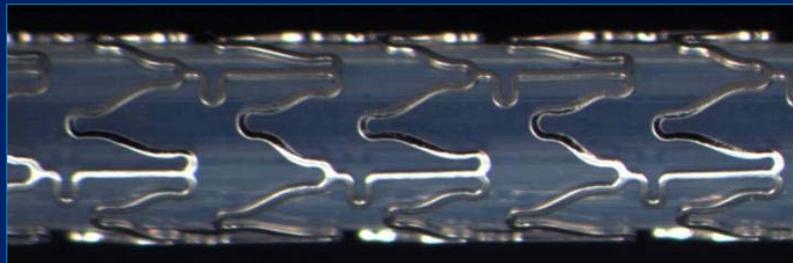

PROMUS Element (PtCr-EES)

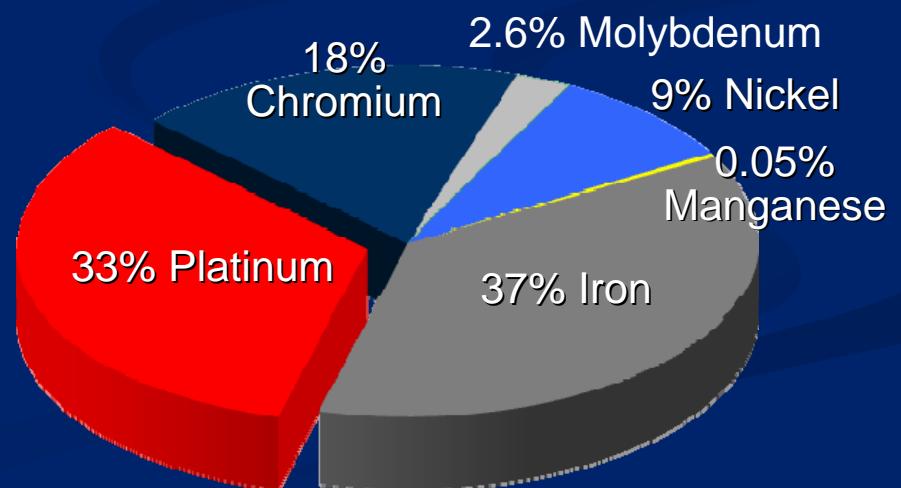


PBMA=poly (n-butyl methacrylate) (primer layer); PVDF-HFP=poly (vinylidene fluoride-co-hexafluoropropylene) (drug matrix layer)


PROMUS Element and PROMUS Stents:

Equivalent Polymer Thickness and Drug Release Profiles

Same Polymer and
Strut Thickness (μm)

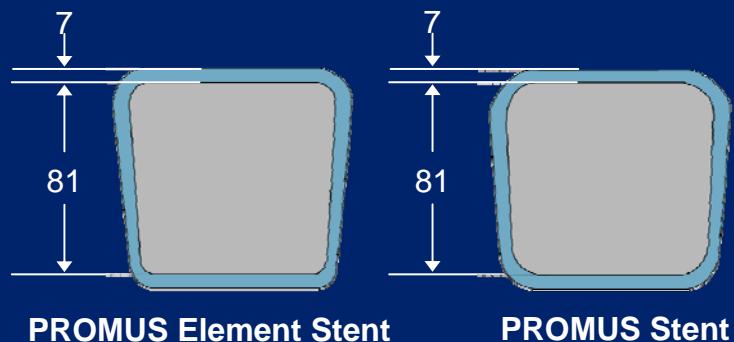

Comparable Kinetic Drug
Release Profiles

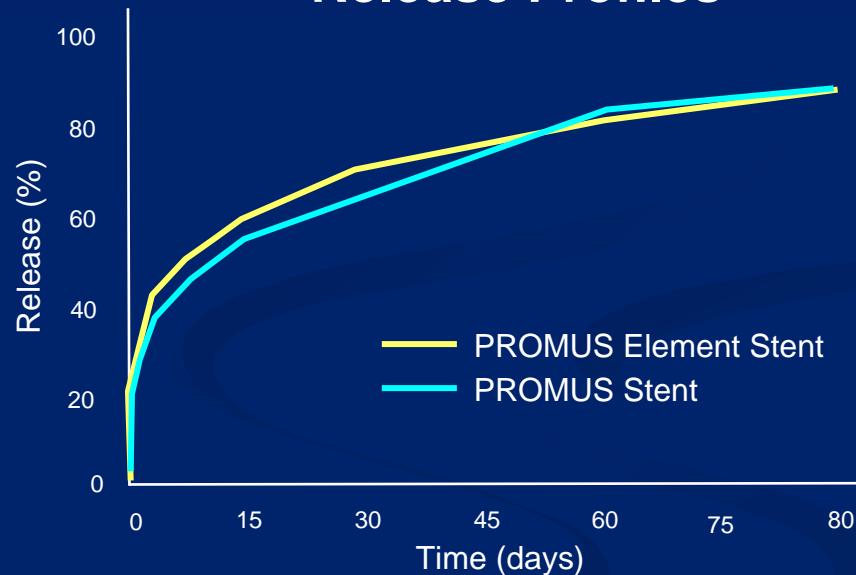


BSC Data on file, average over all sizes, PROMUS Stent 2.5mm x 8mm N=12, 3.0mm x 16mm N=6, 4.0mm x 28mm N=6, PROMUS Element Stent 2.5mm x 8mm N=12, 3.0mm x 15mm N=6, 4.0mm x 28mm N=6.

Drug Release Kinetics In Vivo





Noninjured Porcine Model



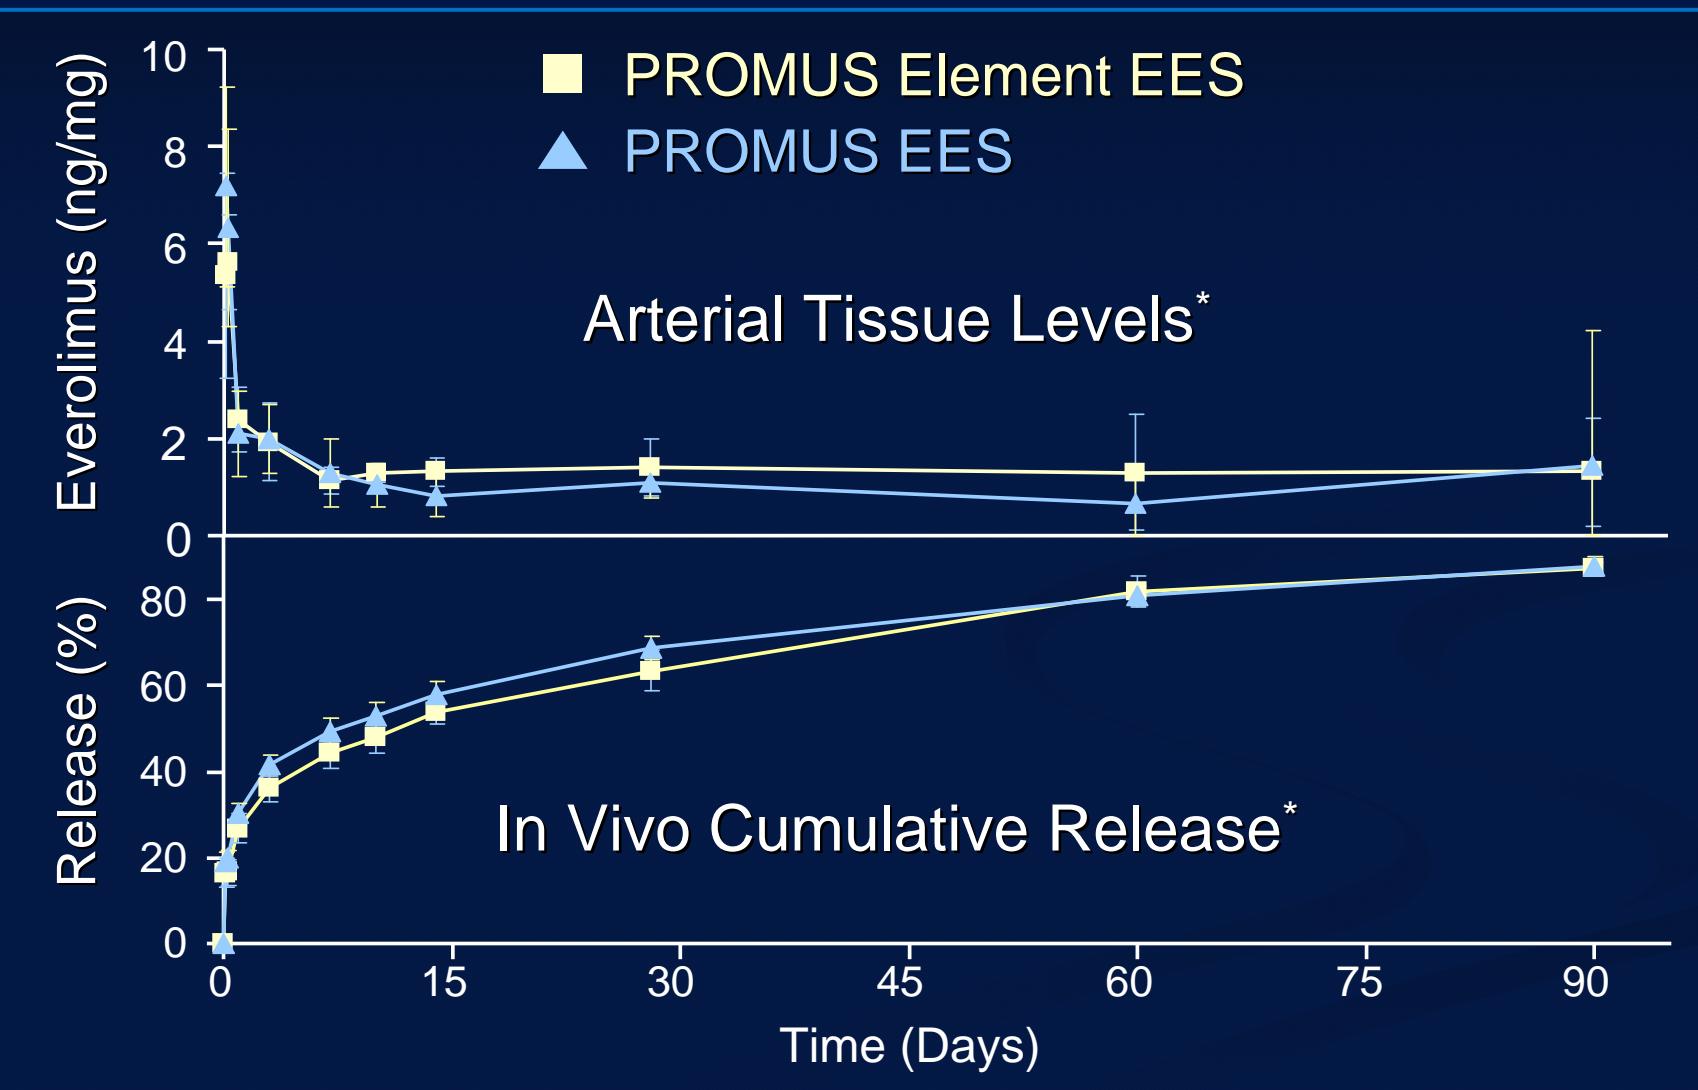


* Boston Scientific Corporation in-house testing; N=9-12 stents per time point; data are mean \pm SD; EES=everolimus-eluting stent

Representative Histology: Porcine Model Stent Overlap Areas @ 30, 90 & 270 Days

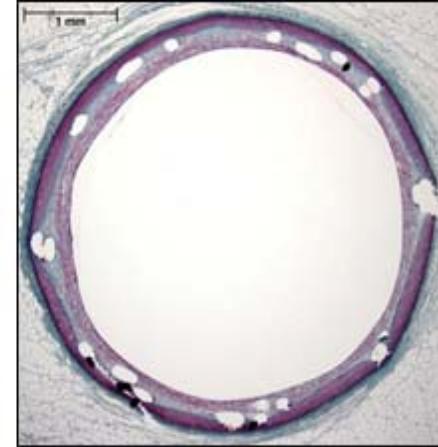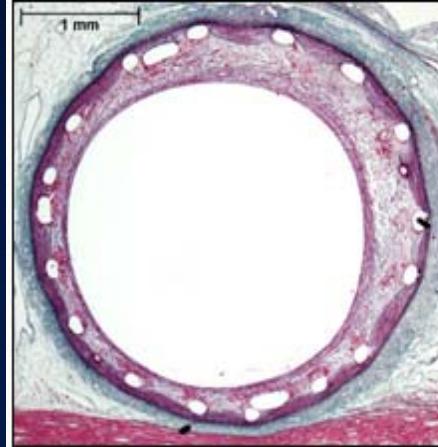

PROMUS
Element

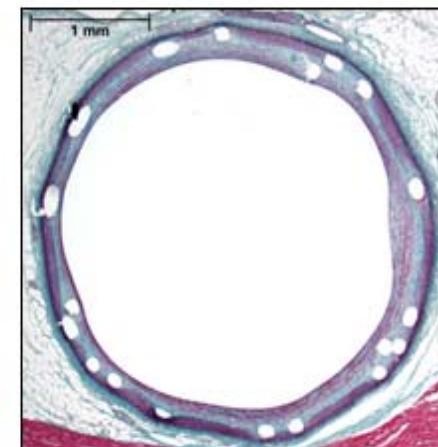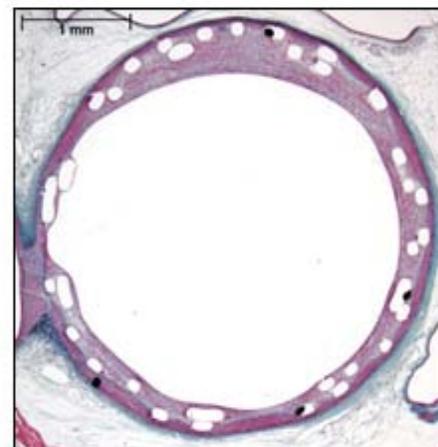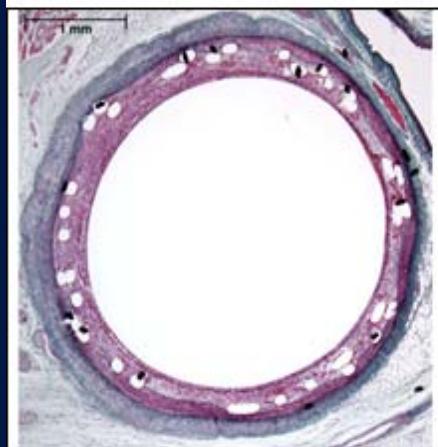

PROMUS
(XIENCE V)

30 Days

90 Days

270 Days

Platinum Chromium Visibility



Cobalt Chromium
0.081mm (0.0032")

Stainless Steel
0.139mm (0.0055")

Platinum Chromium
0.081mm (0.0032")

Cobalt Nickel
0.091mm (0.0036")


Stainless Steel
0.096mm (0.0038")

Radiopacity of a 0.081mm (0.0032") PtCr stent compared to Cobalt Nickel, Cobalt Chromium and Stainless Steel stents.

Data on file Boston Scientific.

PtCr Stent Platform

Radial Strength Bench Test Data

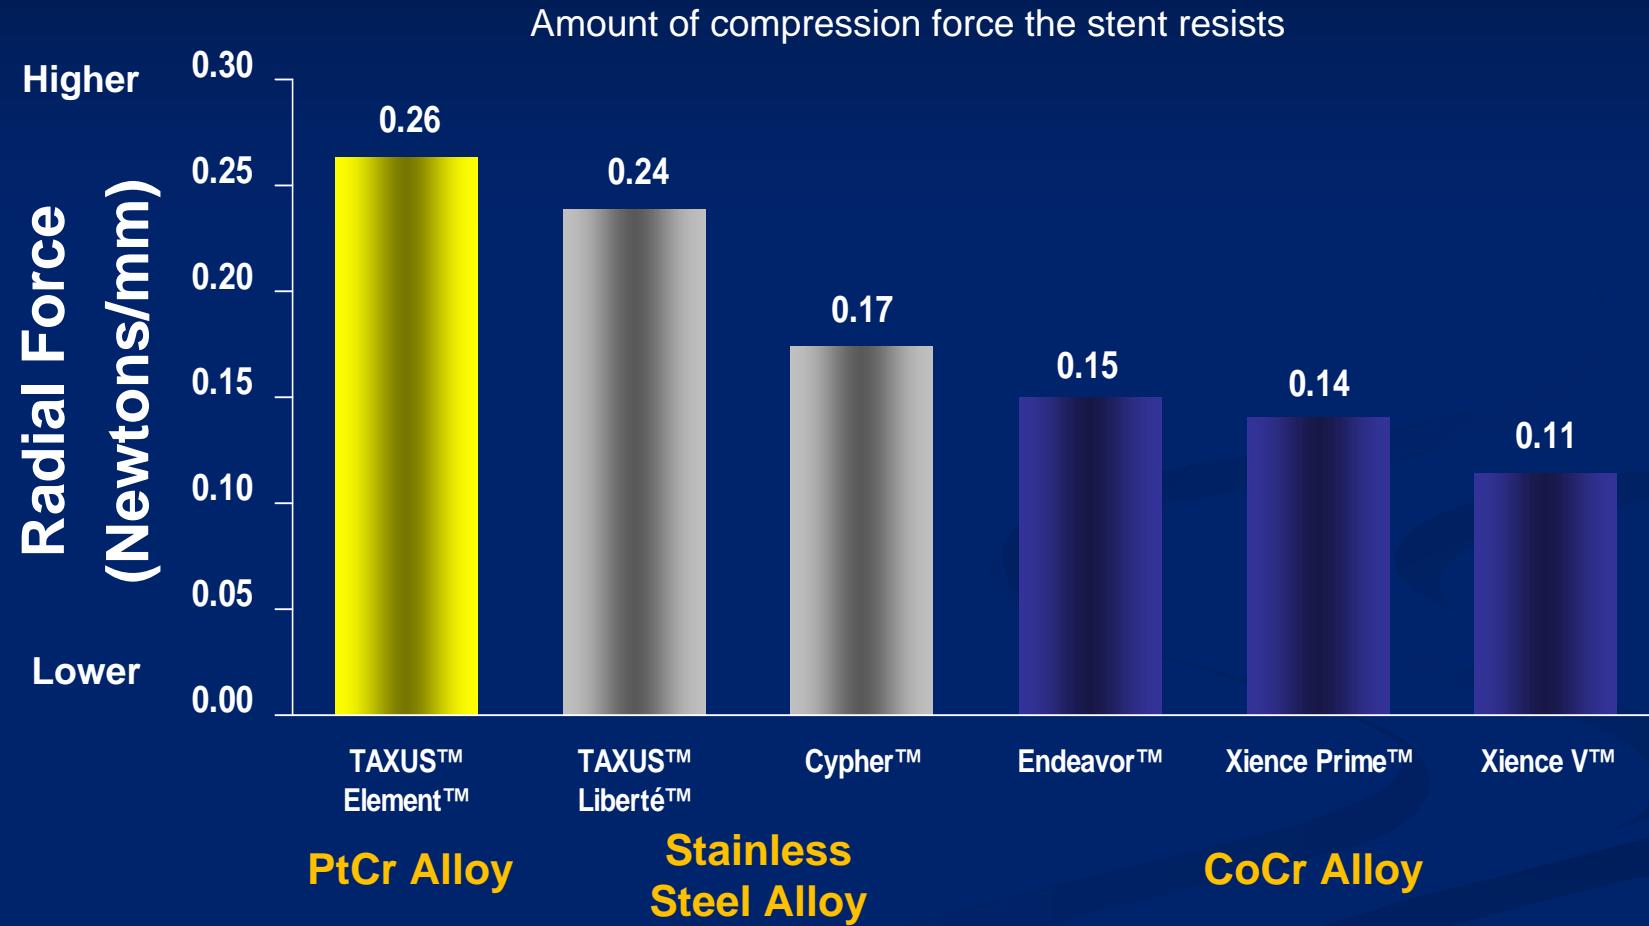


Data on File Boston Scientific. 2.50mm Stents. TAXUS Element n=15. TAXUS Liberté n=10. Cypher n=3.
Xience Prime n=5. Endeavor n=7. Xience V n=10.

PtCr Stent Platform

Recoil Bench Test Data




Percentage stent diameter decreases after balloon deflation

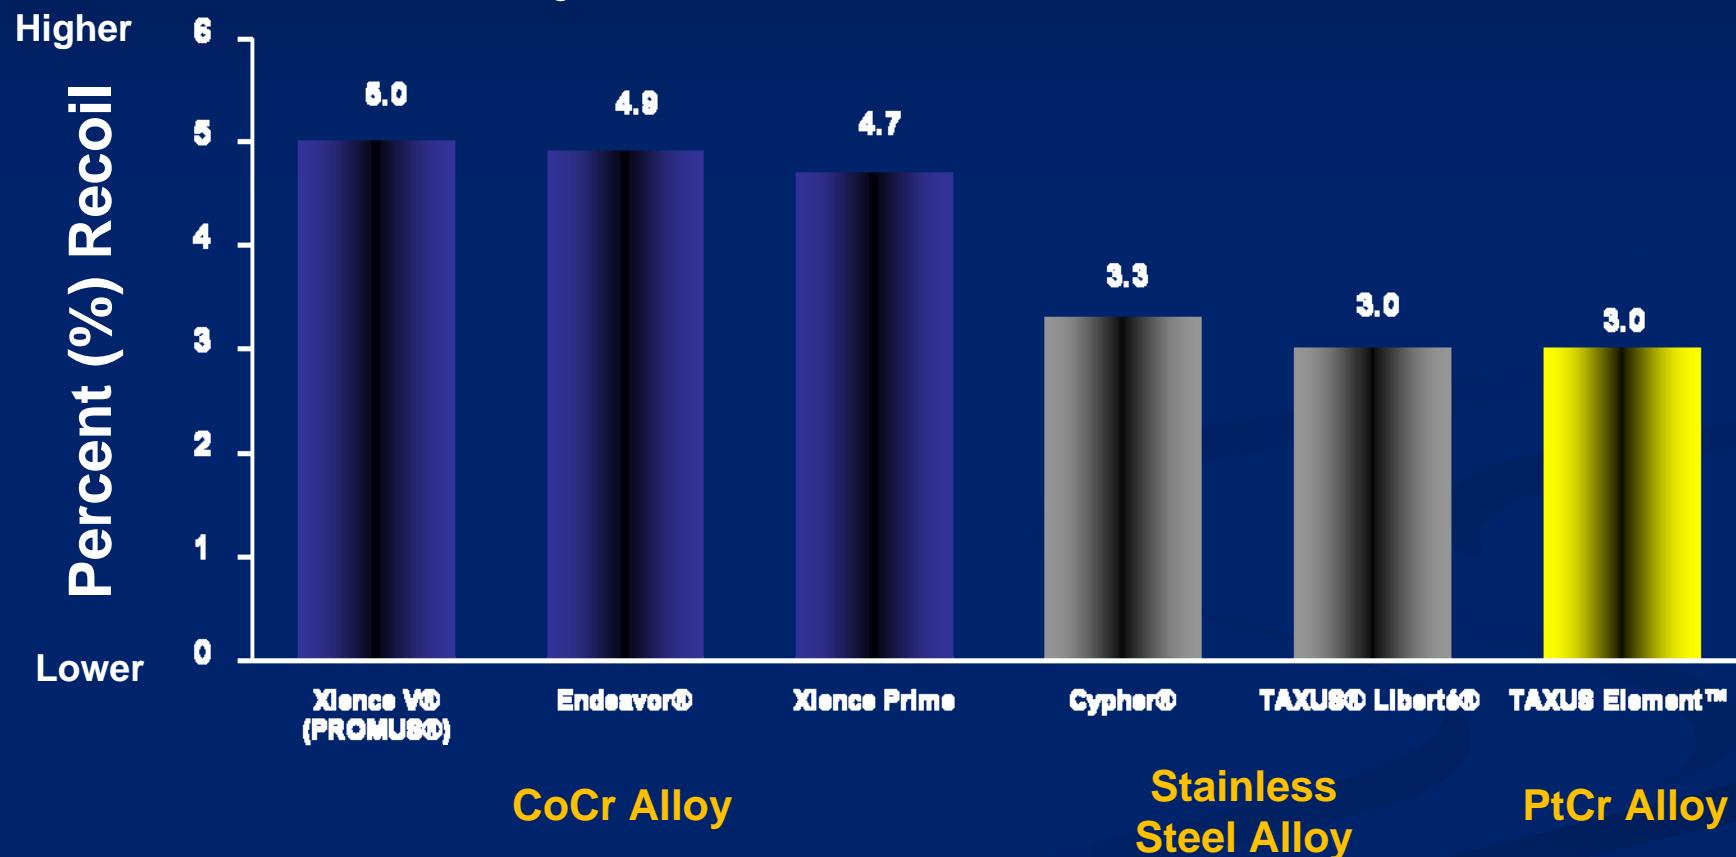

Data on File Boston Scientific. 2.50mm Stents. TAXUS Element n=21. TAXUS Liberté n=6. Cypher n=3.
Xience Prime n=5. Endeavor n=7.

PtCr Stent Platform

Conformability Bench Test Data

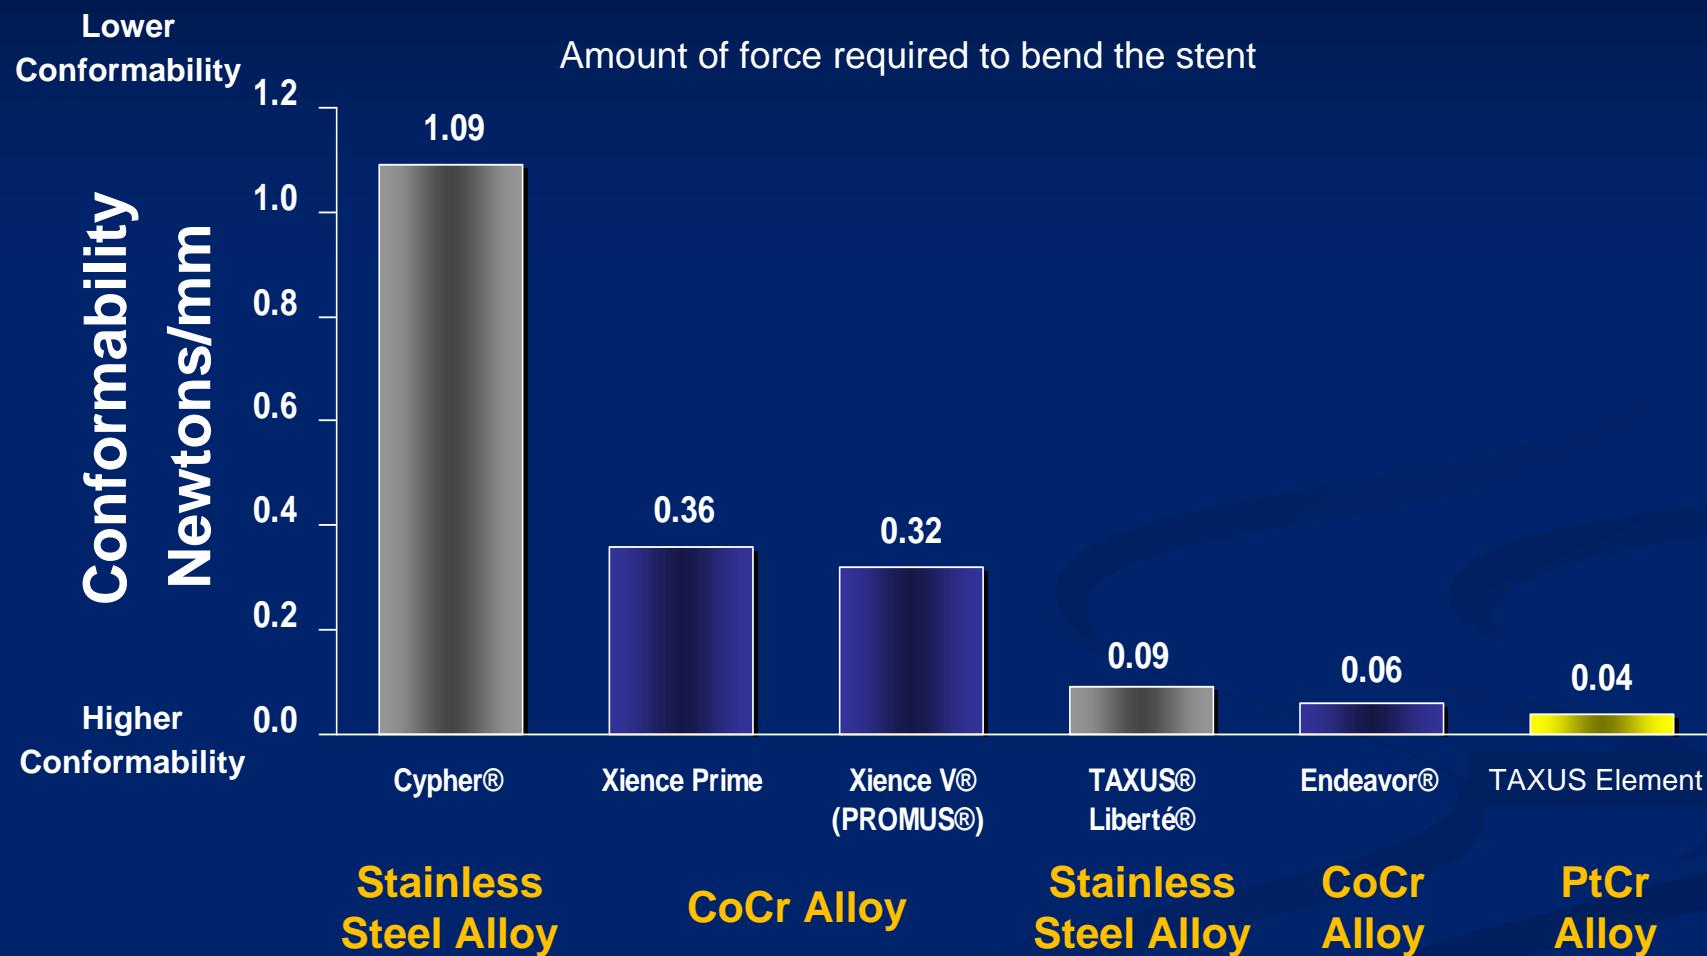

Data on File Boston Scientific. 2.50mm Stents. TAXUS Element n=15. TAXUS Liberté n=15. Cypher n=6.
 Xience Prime n=5. Endeavor n=7. Xience V n=10.


CoCr & PtCr Everolimus-Eluting Stents



Parameter (3.0 mm stents)	CoCr-EES (n=10)	PtCr-EES (n=15)
Strut width (μm)	91	86
Strut thickness (μm)	81	81
Radial strength (N/mm)	0.14	0.23
Stent recoil (%)	4.6	3.6
Conformability (N·mm) [†]	0.30	0.09
Radiopacity/density (g/cm ³)	9.1	9.9
Trackability (gr· cm cath.) [‡]	158	133

[†] Describes stent's ability to match natural vessel curvature without causing vessel straightening; a lower value reflects better conformability; [‡] Amount of work required to pass stent through a tortuous artery model; less work reflects better trackability; 16 mm PtCr-EES & 18 mm CoCr-EES, n=10 per group. N/mm=Newtons per millimeter; N-mm=Newton millimeters

Fracture Resistance & Strut Thickness Element Stent Platform

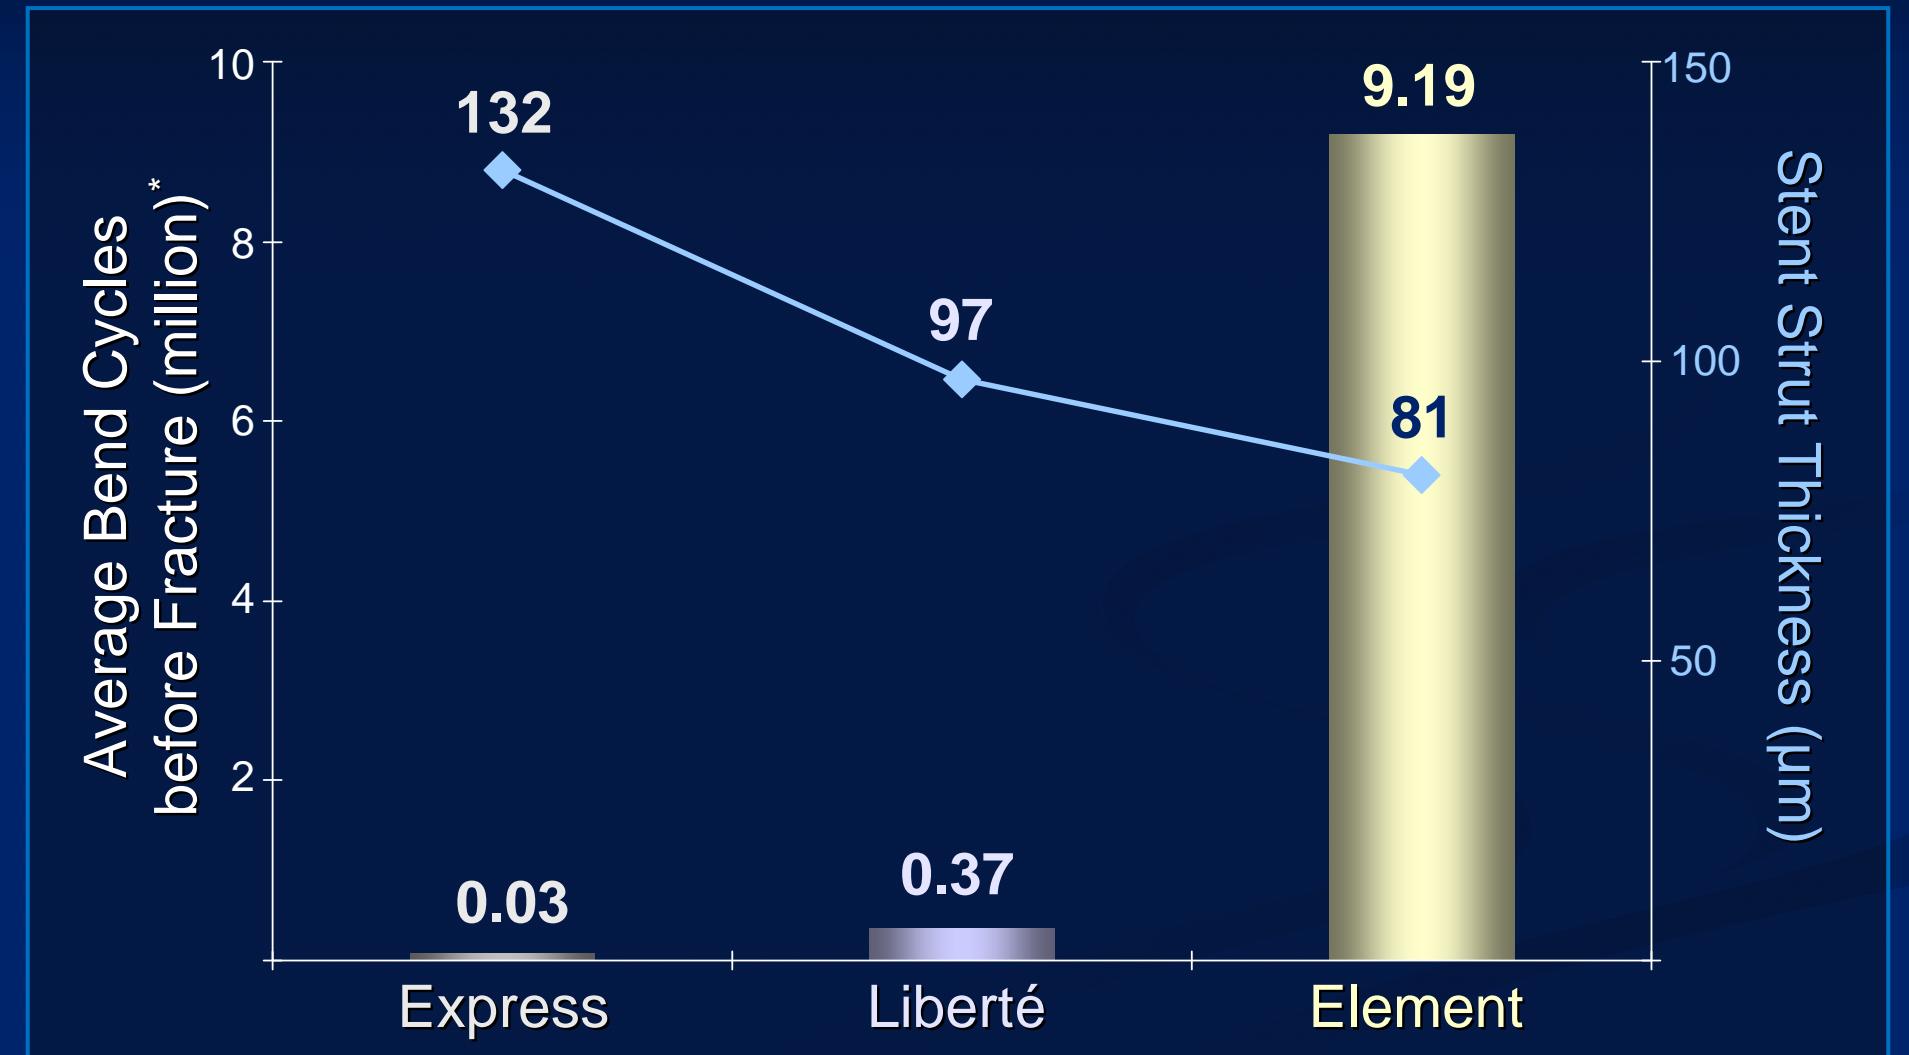

* Boston Scientific Corporation in-house testing; N=20 per stent type

PLATINUM Clinical Trial Program



Study	Design	Primary Endpoint
Pharmacokinetics US, Japan N=22 (5 sites)	Multicenter; Single Arm PROMUS Element EES	Observational
PLATINUM QCA Asia Pacific N=100 (14 sites)	Multicenter; Single Arm PROMUS Element EES	Cardiac Death, MI, TLR, ST at 30 Days
Workhorse RCT US, EU, Japan, AP N=1,530 (132 sites)	Multicenter; 1:1 Randomization PROMUS Element EES; PROMUS EES	12-Month TLF
Small Vessel US, EU, Japan, AP N=94 (23 sites)	Multicenter; Single Arm PROMUS Element EES	12-Month TLF
Long Lesion US, EU, Japan, AP N=102 (30 sites)	Multicenter; Single Arm PROMUS Element EES	12-Month TLF

AP=Asia Pacific; MI=myocardial infarction; EES=everolimus-eluting stent; QCA=quantitative coronary angiography; RCT=randomized controlled trial; ST=stent thrombosis; TLF=target lesion failure; TLR=target lesion revascularization

PLATINUM Clinical Trial Program



Study	Design	Primary Endpoint
Pharmacokinetics US, Japan N=22 (5 sites)	Multicenter; Single Arm PROMUS Element EES	Observational
PLATINUM QCA Asia Pacific N=100 (14 sites)	Multicenter; Single Arm PROMUS Element EES	Cardiac Death, MI, TLR, ST at 30 Days
Workhorse RCT US, EU, Japan, AP N=1,530 (132 sites)	Multicenter; 1:1 Randomization PROMUS Element EES; PROMUS EES	12-Month TLF
Small Vessel US, EU, Japan, AP N=94 (23 sites)	Multicenter; Single Arm PROMUS Element EES	12-Month TLF
Long Lesion US, EU, Japan, AP N=102 (30 sites)	Multicenter; Single Arm PROMUS Element EES	12-Month TLF


AP=Asia Pacific; MI=myocardial infarction; EES=everolimus-eluting stent; QCA=quantitative coronary angiography; RCT=randomized controlled trial; ST=stent thrombosis; TLF=target lesion failure; TLR=target lesion revascularization

PLATINUM QCA

Pre-specified Efficacy Endpoint



In-Stent Late Loss at 9 Months – Workhorse Lesions

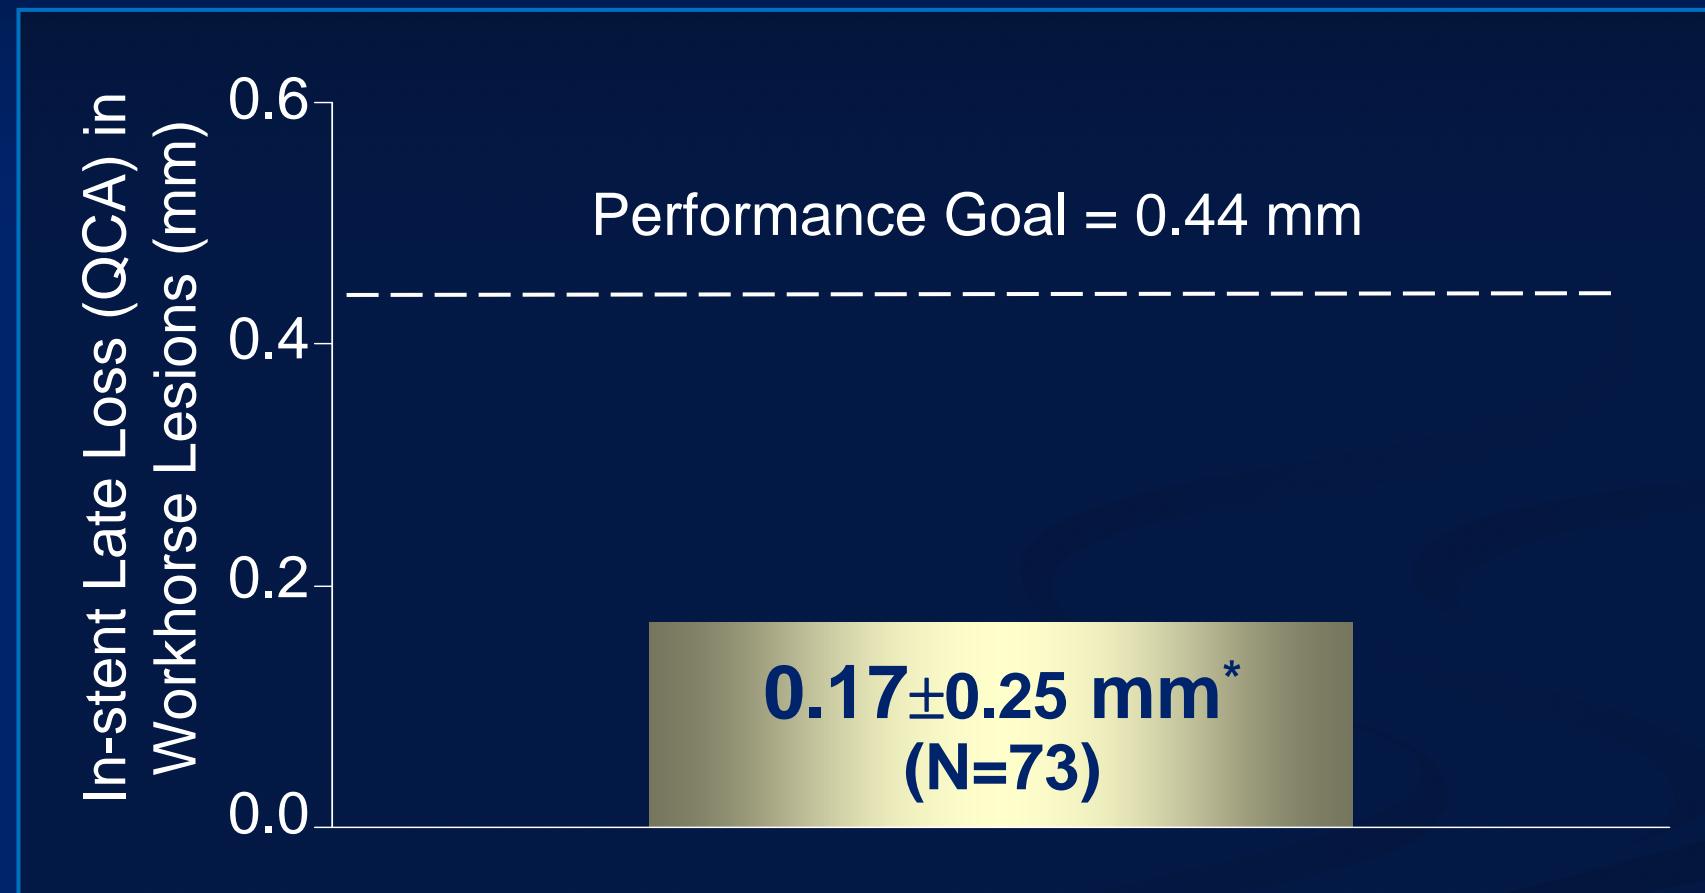

Workhorse lesions: RVD $\geq 2.5 - \leq 4.25$ mm, lesion length ≤ 24 mm

* Mean \pm SD; value of 0.17 with an upper confidence bound of 0.22 mm is significantly less ($P < 0.001$) than performance goal based on historical TAXUS Express value (0.41 mm + delta [0.03 mm]).

PLATINUM QCA: In-stent Late Loss PROMUS Element & PROMUS



Study	In-Stent Late Loss (mm)	Time Point (months)
PLATINUM QCA (Workhorse lesions*)	0.17 ± 0.25 (n=73)	9
SPIRIT First [†]	0.10 ± 0.21 (n=23)	6
	0.24 ± 0.27 (n=20)	12
SPIRIT II [‡]	0.11 ± 0.27 (n=237)	6
SPIRIT III [¶]	0.16 ± 0.41 (n=301)	8


* Workhorse lesions: (RVD $\geq 2.5 - \leq 4.25$ mm, lesion length ≤ 24 mm; [†] Serruys, et al. *EuroIntervention* 2005;1:58 & Tsuchida, et al. *EuroIntervention* 2005;1:266; [‡]Serruys, et al. *EuroIntervention* 2006;2:286; [¶]Stone, et al. *JAMA* 2008;299:1903.

PLATINUM QCA: IVUS Outcomes

PLATINUM QCA Study




■ Post-Procedure ■ 9 Months

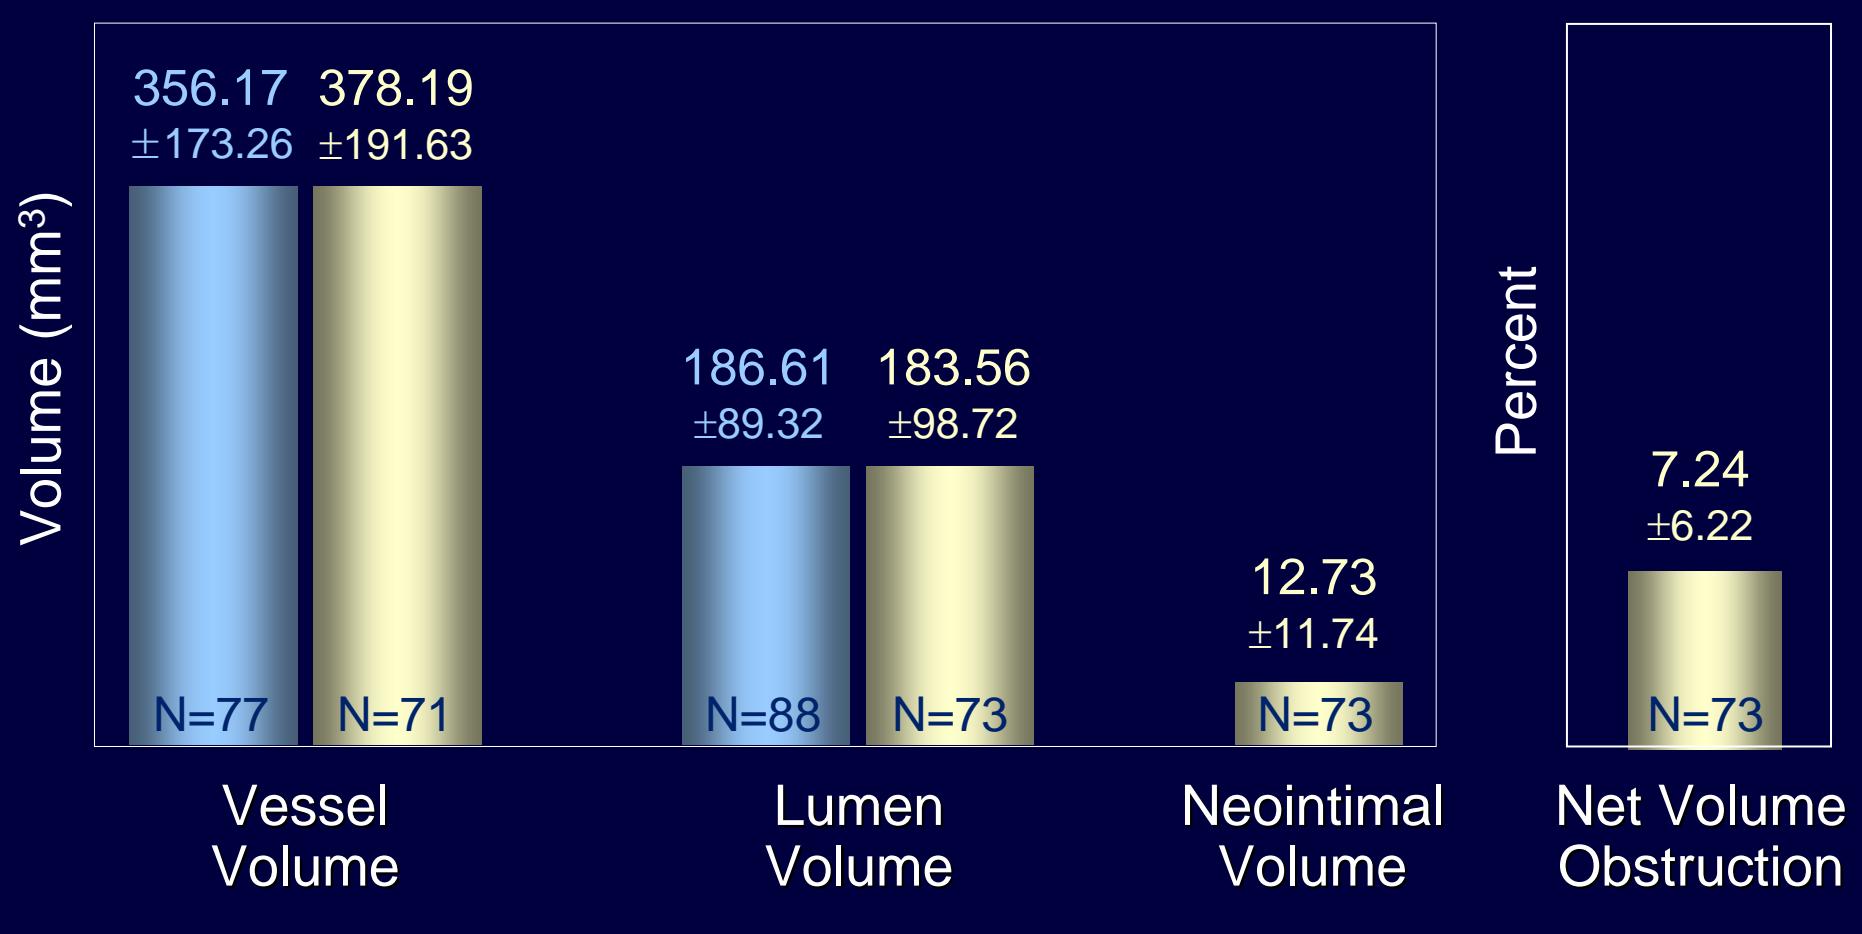

PLATINUM QCA

Pre-specified IVUS Efficacy Endpoint

Incomplete Stent Apposition Post Procedure

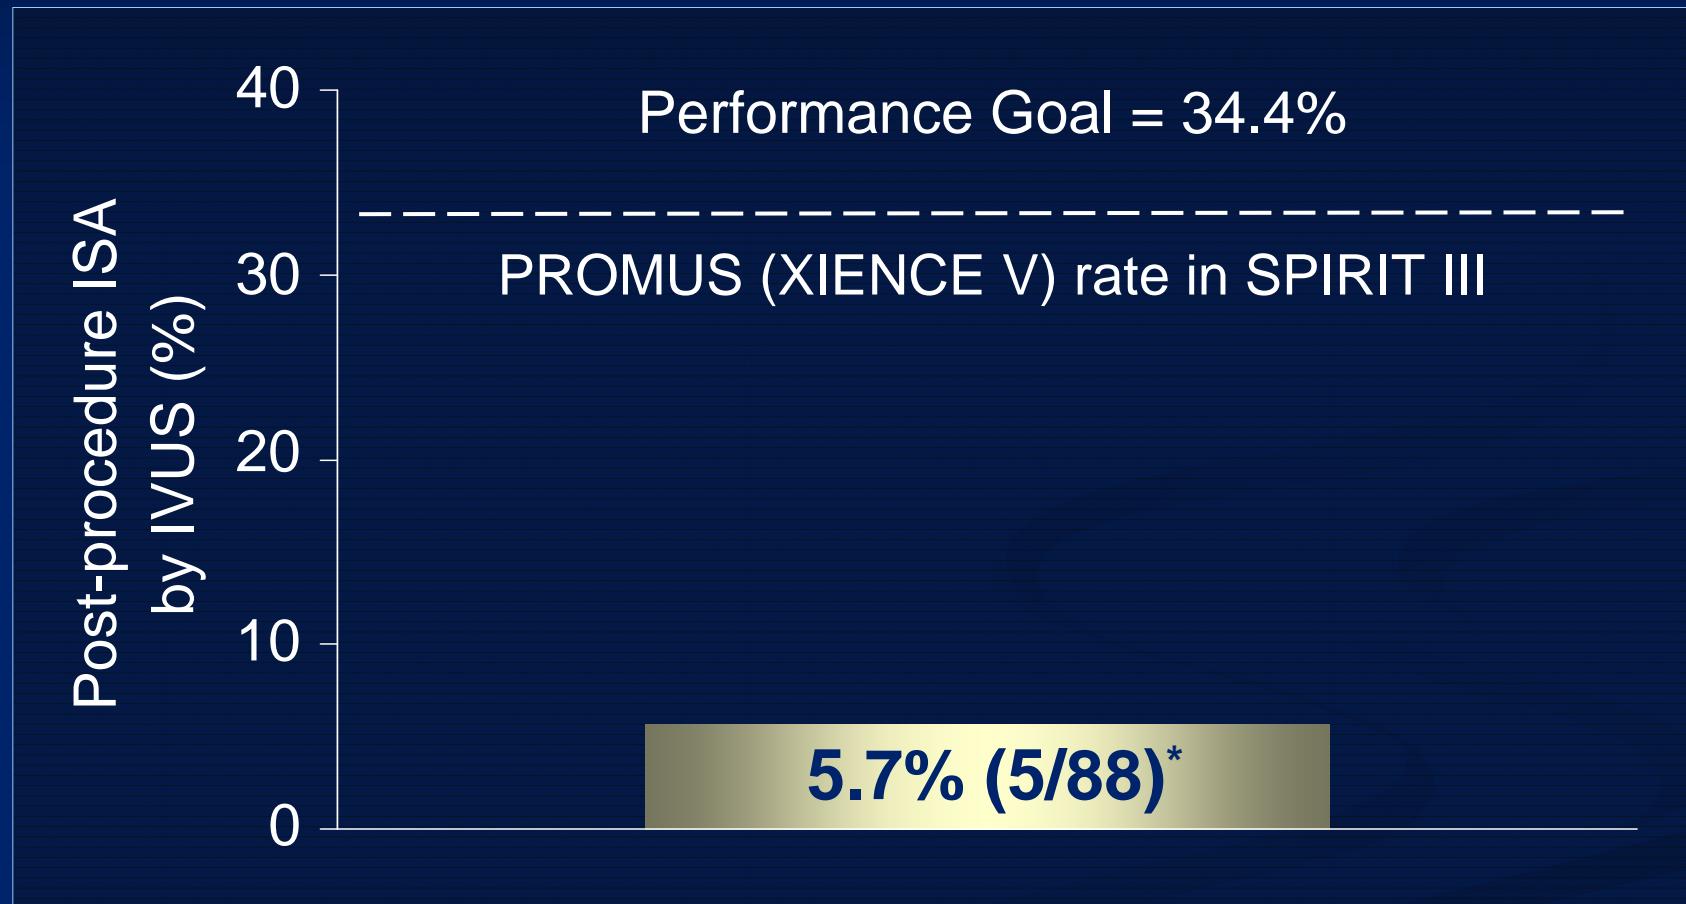

* 12 patients had unreadable post-procedure analyses; value of 5.7% with upper confidence bound of 11.6% is significantly below ($P<0.001$) the performance goal of 34.4% post-procedure ISA based on PROMUS (XIENCE V) data from SPIRIT III (Stone, et al. JAMA. 2008;299:1903)
ISA=incomplete stent apposition

Meredith I. TCT2010.

Incomplete Stent Apposition (IVUS)



PLATINUM QCA Study

Event	Patients (N=69)* (Post-procedure & 9M)
Early (Post-Procedure)	5.8% (4)
Late (9-Month)	0.0% (0)
Resolved	5.8% (4)
Persistent	0.0% (0)
Late Acquired	0.0% (0)

* Patients with both post-procedure and 9-month assessments

Clinical Outcomes through 9 Months



PLATINUM QCA (N=100)	30 Days	9 Months
All death, MI, TVR	1.0% (1)	1.0% (1)
All death	0.0% (0)	0.0% (0)
Myocardial infarction	0.0% (0)	0.0% (0)
Q-wave	0.0% (0)	0.0% (0)
Non-Q-wave	0.0% (0)	0.0% (0)
Target vessel revascularization	1.0% (1)	1.0% (1)
Target lesion revascularization	1.0% (1)	1.0% (1)
Target lesion failure*	1.0% (1)	1.0% (1)
Stent thrombosis (ARC def/prob)	1.0% (1)	1.0% (1)

* Ischemia-driven TLR, or MI/cardiac death related to the target vessel

Meredith I. TCT2010.

PLATINUM Clinical Trial Program




Study	Design	Primary Endpoint
Pharmacokinetics US, Japan N=22 (5 sites)	Multicenter; Single Arm PROMUS Element EES	Observational
PLATINUM QCA Asia Pacific N=100 (14 sites)	Multicenter; Single Arm PROMUS Element EES	Cardiac Death, MI, TLR, ST at 30 Days
Workhorse RCT US, EU, Japan, AP N=1,530 (132 sites)	Multicenter; 1:1 Randomization PROMUS Element EES; PROMUS EES	12-Month TLF
Small Vessel US, EU, Japan, AP N=94 (23 sites)	Multicenter; Single Arm PROMUS Element EES	12-Month TLF
Long Lesion US, EU, Japan, AP N=102 (30 sites)	Multicenter; Single Arm PROMUS Element EES	12-Month TLF

AP=Asia Pacific; MI=myocardial infarction; EES=everolimus-eluting stent; QCA=quantitative coronary angiography; RCT=randomized controlled trial; ST=stent thrombosis; TLF=target lesion failure; TLR=target lesion revascularization

PLATINUM Trial Algorithm



Patients with 1 or 2 *de novo* native coronary artery target lesions
RVD ≥ 2.5 to ≤ 4.25 ; Lesion length ≤ 24 mm



Peri-proc: ASA ≥ 300 mg,
clopidogrel ≥ 300 mg load unless on
chronic Rx

Randomized 1:1

Stratified by diabetes, intention to treat 1 vs. 2 target lesions, & study site

Cobalt chromium
everolimus-eluting stent

Platinum chromium
everolimus-eluting stent

ASA indefinitely, thienopyridine ≥ 6 mos (≥ 12 mos if not high risk for bleeding)

Clinical f/u only: 1, 6, 12, 18 months then yearly for 2-5 years

PLATINUM Major Endpoints




- ◆ Primary endpoint
 - ◆ Target lesion failure (TLF) at 12 months
 - Cardiac death related to the target vessel, or
 - MI related to the target vessel, or
 - Ischemia-driven target lesion revascularization
 - ◆ Per protocol population*
- ◆ Additional endpoints
 - ◆ Components of TLF
 - ◆ Stent thrombosis (ARC definite/probable)
 - ◆ Technical success†
 - ◆ Clinical procedural success‡

* Patients who received ≥ 1 assigned study stent

† Successful delivery & deployment of study stent to the target vessel, without balloon rupture or stent embolization

‡ Lesion DS<30% with visually assessed TIMI 3 flow and without the occurrence of in-hospital cardiac death, MI, or TVR

Patient Flow

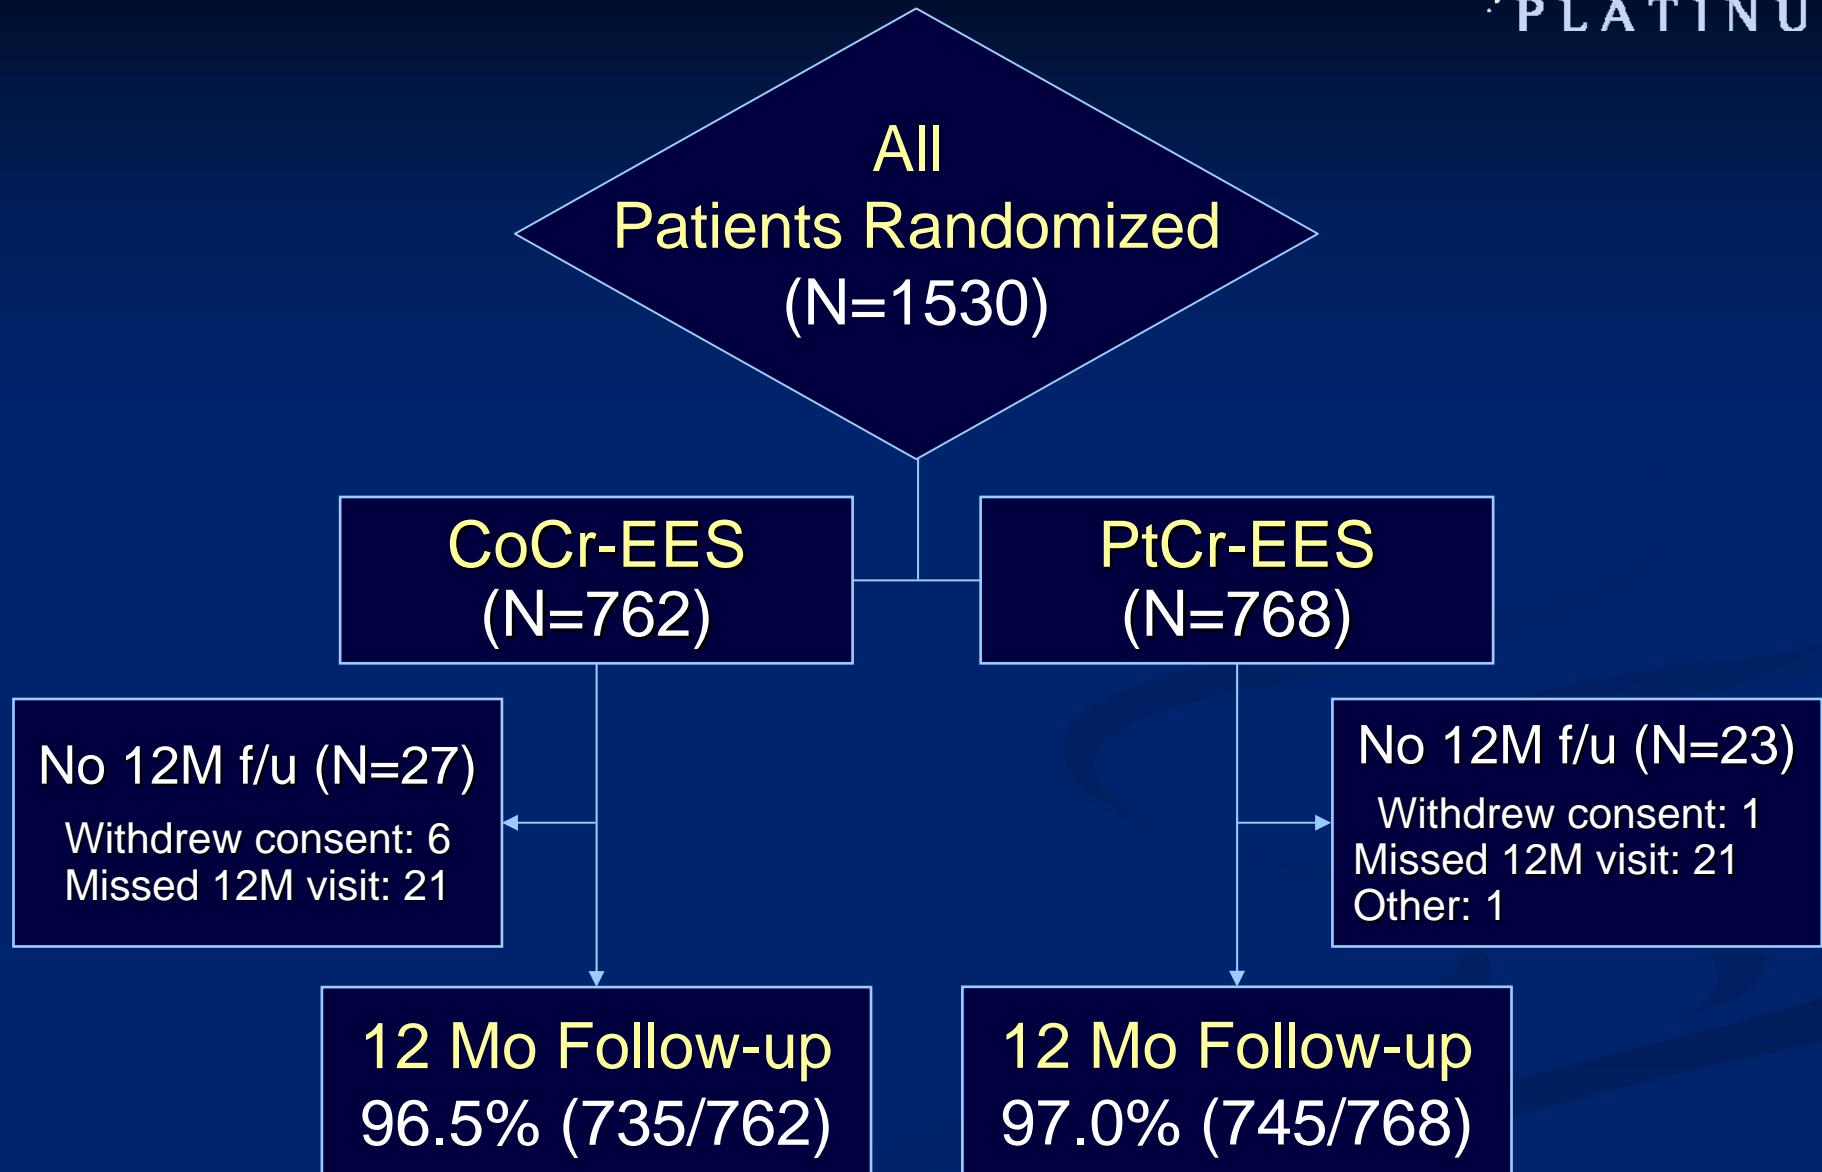

Baseline Demographics



	CoCr-EES (N=762)	PtCr-EES (N=768)	<i>P</i> value
Age, years	63.1 ± 10.3	64.0 ± 10.3	0.09
Male	71.1%	71.6%	0.83
Hypertension	73.2%	70.9%	0.32
Hyperlipidemia	76.2%	78.2%	0.36
Diabetes	25.1%	22.0%	0.16
- Insulin treated	6.3%	7.7%	0.29
Current smoker	17.7%	21.0%	0.10
Prior MI	21.1%	21.0%	0.99
Unstable angina	24.7%	24.1%	0.80

Baseline Lesion Characteristics (QCA)



	CoCr-EES (N=762 Patients) (N=841 Lesions)	PtCr-EES (N=768 Patients) (N=853 Lesions)	<i>P</i> value
Target lesions	1.10 ± 0.31	1.11 ± 0.31	0.66
- 2 lesions treated	10.1%	11.1%	0.54
RVD, mm	2.63 ± 0.49	2.67 ± 0.49	0.09
MLD, mm	0.74 ± 0.34	0.75 ± 0.35	0.40
DS, %	71.9 ± 11.5	71.8 ± 11.5	0.87
Lesion length, mm	12.5 ± 5.5	13.0 ± 5.7	0.10

Procedural Characteristics



	CoCr-EES (N=762 Patients) (N=841 Lesions)	PtCr-EES (N=768 Patients) (N=853 Lesions)	<i>P</i> value
Stents per patient	1.20 ± 0.48	1.16 ± 0.44	0.16
Stents per target lesion	1.08 ± 0.35	1.05 ± 0.26	0.01
Max stent diam. per lesion (mm)	3.05 ± 0.44	3.09 ± 0.45	0.07
Stent length per lesion (mm)	19.7 ± 8.9	20.5 ± 7.0	0.06
Post-dilatation	49.3%	49.8%	0.84
Max pressure overall (atm)	15.9 ± 3.2	16.3 ± 3.1	0.002
Fluoroscopy time (min)	11.3 ± 10.1	12.2 ± 11.8	0.10

Technical & Procedural Success



	CoCr-EES (N=762)	PtCr-EES (N=768)	<i>P</i> value
Technical success ^a	98.8%	99.4%	0.14
Clinical procedural success ^b	98.2%	98.3%	0.83
Unplanned (bail-out) stenting ^c	9.8%	5.9%	0.004
- Procedural complications	4.7%	3.8%	0.36
- Inadequate lesion coverage	3.4%	1.4%	0.01
- Other reasons	1.7%	0.7%	0.06

a: Successful delivery & deployment of study stent to the target vessel, without balloon rupture or stent embolization (per stent)

b: Mean lesion diameter stenosis <30% with visually assessed TIMI 3 flow and without the occurrence of in-hospital cardiac death, MI, or TVR

c: Study or non-study stents

Post-Procedure Angiographic Outcomes



	CoCr-EES (N=762 Patients) (N=841 Lesions)	PtCr-EES (N=768 Patients) (N=853 Lesions)	<i>P</i> value
RVD, mm	2.67 ± 0.50	2.70 ± 0.49	0.27
MLD, in-stent, mm	2.54 ± 0.44	2.57 ± 0.42	0.25
MLD, in-segment, mm	2.16 ± 0.47	2.19 ± 0.47	0.15
DS, in-stent, %	4.3 ± 8.7	4.3 ± 9.1	0.95
DS, in-segment, %	19.2 ± 9.0	18.8 ± 8.6	0.43
Acute gain, in-stent, mm	1.80 ± 0.45	1.81 ± 0.43	0.73
Acute gain, in-segment, mm	1.42 ± 0.47	1.44 ± 0.46	0.45

Antiplatelet Medication Usage




Medication	CoCr-EES (N=762)	PtCr-EES (N=768)	P value
Pre-PCI*			
Aspirin	99.6%	99.3%	0.73
Thienopyridine	98.6%	99.0%	0.48
Aspirin + Thienopyridine	98.3%	98.3%	0.98
Discharge			
Aspirin	99.6%	98.7%	0.053
Thienopyridine	99.1%	98.8%	0.63
Aspirin + Thienopyridine	98.8%	97.7%	0.08
12 Months			
Aspirin	97.4%	97.6%	0.84
Thienopyridine	89.4%	90.9%	0.34
Aspirin + Thienopyridine	87.3%	89.3%	0.26

*Per-protocol, thienopyridine could be given up to 2 hours after the procedure

Primary Endpoint




Target Lesion Failure at 12 Months

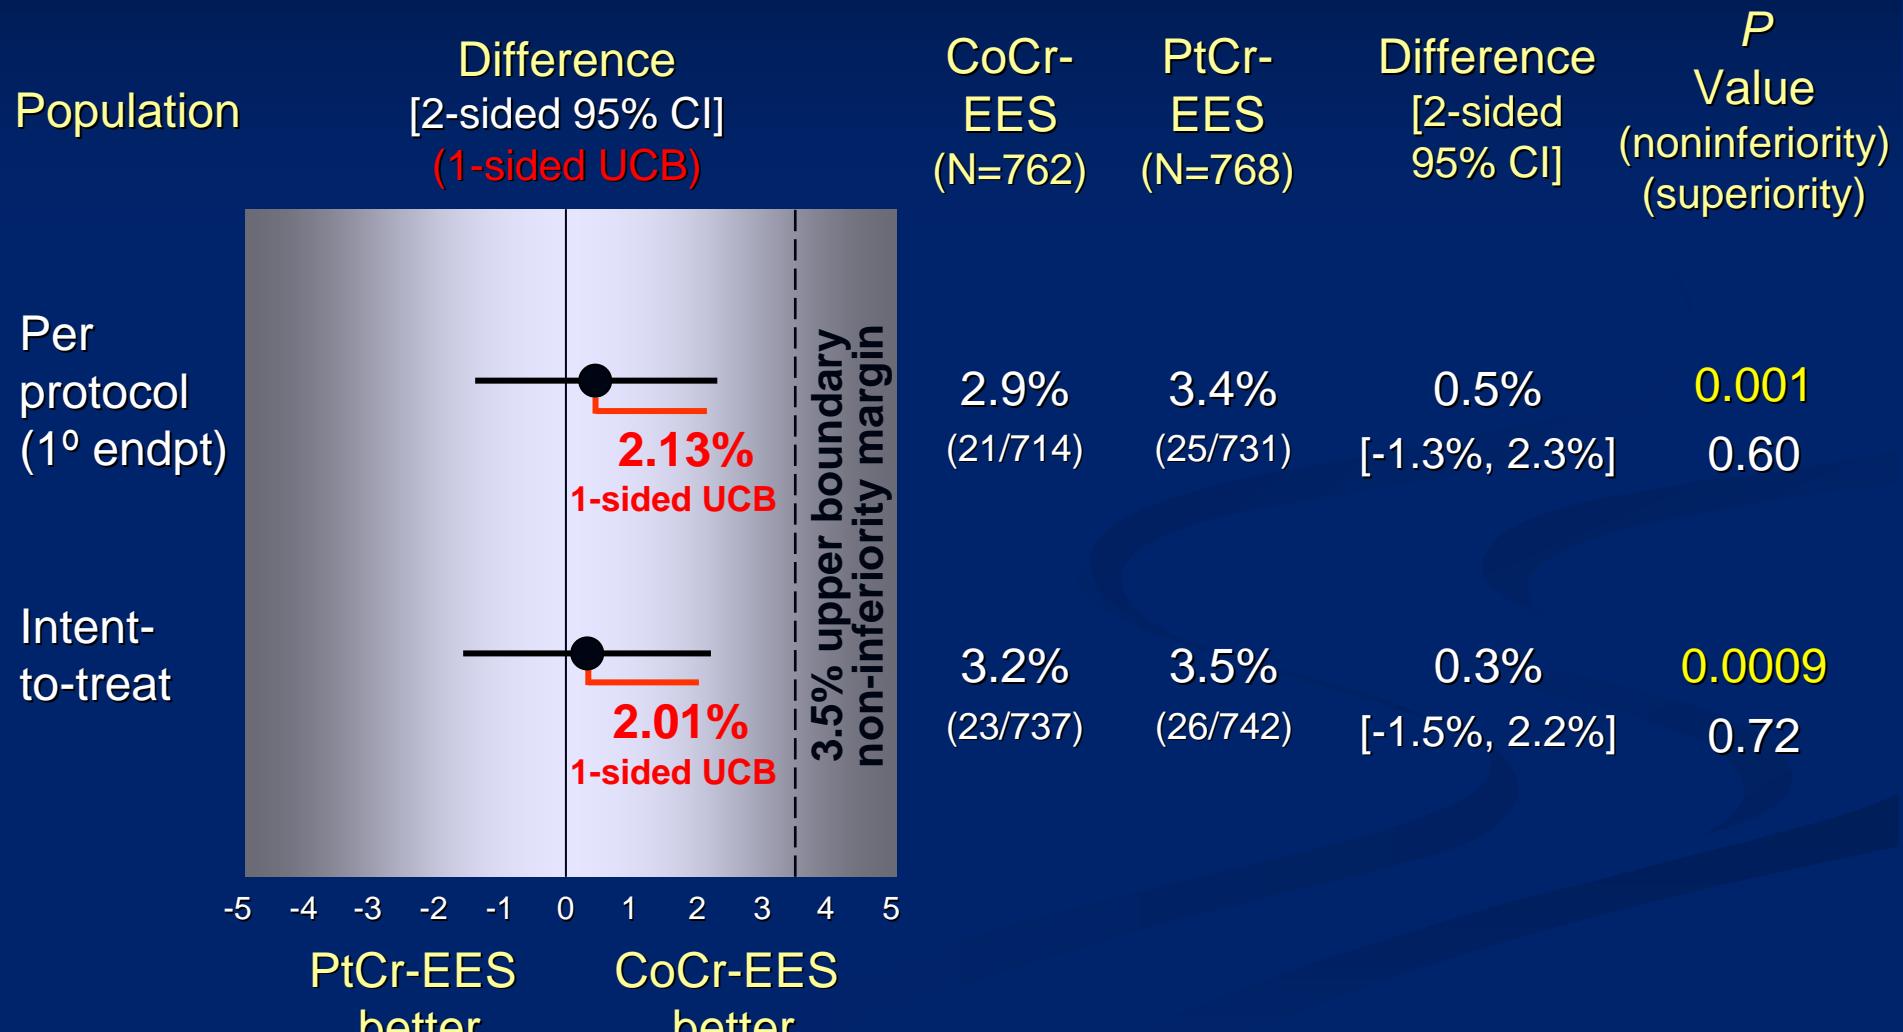

Target Lesion Failure

Time-to-event analysis

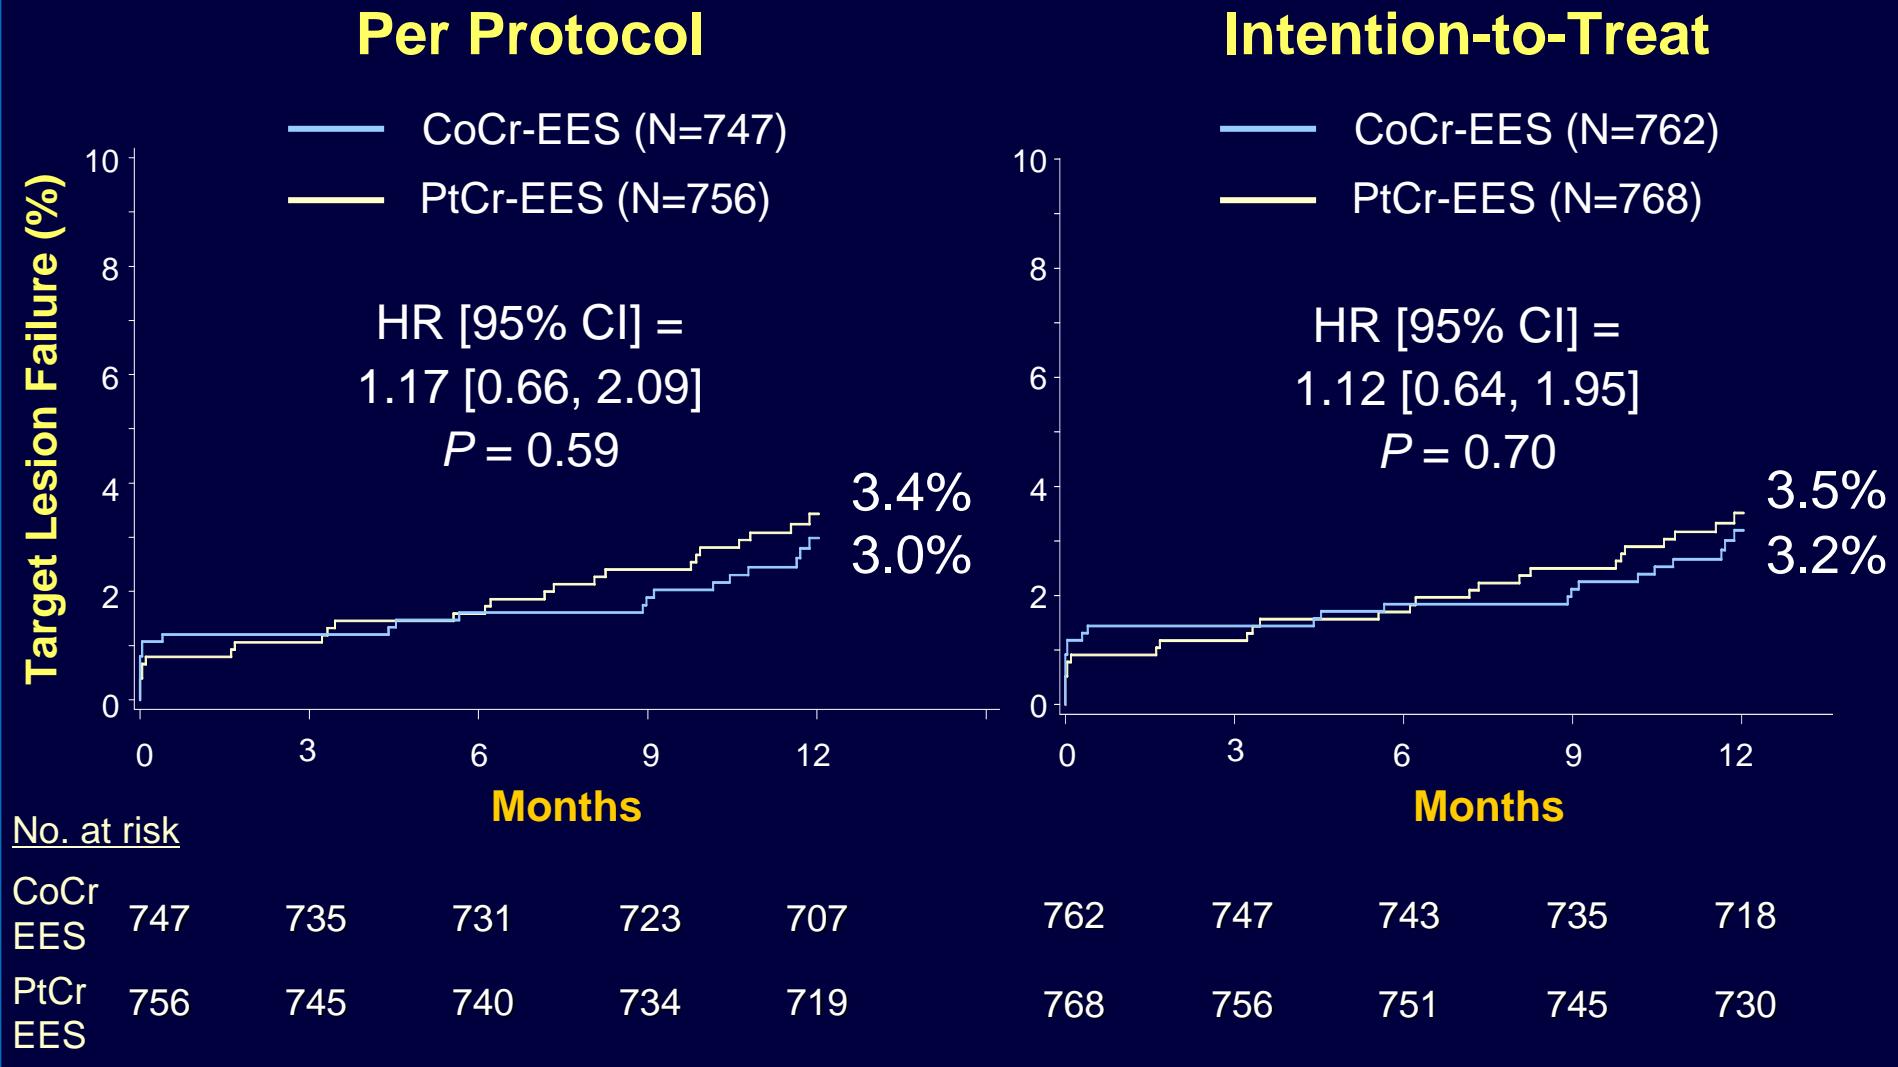

Target Lesion Failure Components

12 Months



Per Protocol

Intention-to-Treat

	CoCr-EES (N=747)	PtCr-EES (N=756)	<i>P</i> value	CoCr-EES (N=762)	PtCr-EES (N=768)	<i>P</i> value
TLF	2.9%	3.4%	0.60	3.2%	3.5%	0.72
Cardiac death-TV	0.4%	0.8%	0.51	0.4%	0.8%	0.51
MI-TV	1.4%	0.7%	0.18	1.6%	0.8%	0.14
ID-TLR	1.8%	1.9%	0.89	1.9%	1.9%	0.96

Death and Myocardial Infarction

12 Months – Intent-to-Treat



	CoCr-EES (N=762)	PtCr-EES (N=768)	P value
All-cause death or MI	3.0%	2.4%	0.49
All-cause death	1.2%	1.3%	0.85
Cardiac	0.7%	0.9%	0.58
Non-cardiac	0.5%	0.4%	0.72
Myocardial Infarction	1.8%	1.1%	0.25
Q-wave	0.7%	0.1%	0.12
Non-Q-wave	1.2%	0.9%	0.59
Cardiac death or MI	2.5%	2.0%	0.56

Revascularization, Ischemia-driven

12 Months – Intent-to-Treat




	CoCr-EES (N=762)	PtCr-EES (N=768)	P value
TVR	2.9%	2.7%	0.83
TLR	1.9%	1.9%	0.96
TLR, PCI	1.6%	1.3%	0.64
TLR, CABG	0.3%	0.5%	0.69
TVR non-TLR	1.1%	0.9%	0.77

Stent Thrombosis – ARC Def/Prob



12 Months – Intent-to-Treat

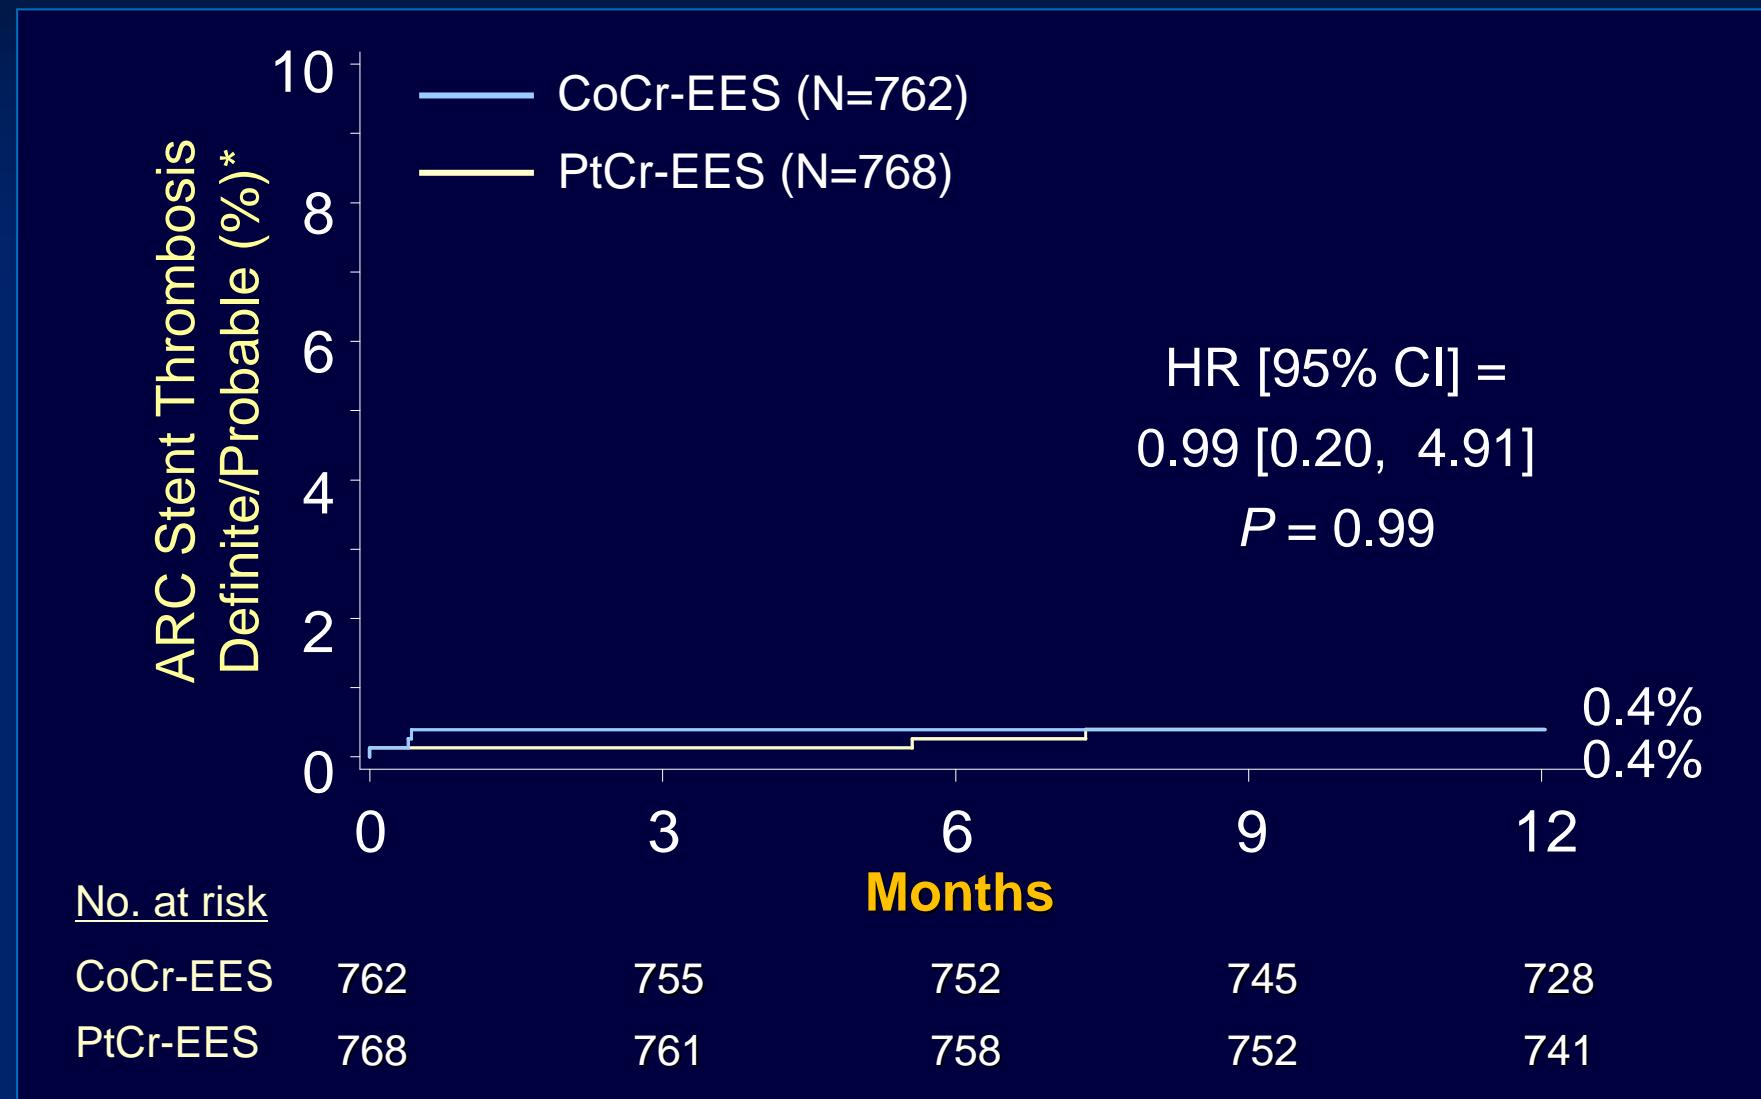

* All were definite ST

Limitations

- ◆ Patients with AMI, CTO, bifurcation, LMCA lesion, SVG lesion, ostial lesions or lesions with thrombus or excessive tortuosity or calcification were excluded
- ◆ Event rates were lower than expected; non-inferiority based on a delta of 3.5% was demonstrated, but small differences between PtCr-EES and CoCr-EES cannot be excluded
- ◆ Trial was not designed to assess differences in deliverability, acute performance or ease of use

Conclusions



- ◆ A novel PtCr-EES has been developed which has been shown to be noninferior to the predicate CoCr-EES for TLF, with non-significant differences in measures of safety and efficacy demonstrated through 12-month follow-up after PCI

The PLATINUM Trial



EXPEDITED PUBLICATION

A Prospective, Randomized Evaluation of a Novel Everolimus-Eluting Coronary Stent

The PLATINUM (A Prospective, Randomized, Multicenter Trial to Assess an Everolimus-Eluting Coronary Stent System [PROMUS Element] for the Treatment of up to Two De Novo Coronary Artery Lesions) Trial

Gregg W. Stone, MD,* Paul S. Teirstein, MD,† Ian T. Meredith, MBBS, PhD,‡ Bruno Farah, MD,§ Christophe L. Dubois, MD, PhD,|| Robert L. Feldman, MD,¶ Joseph Dens, MD, PhD,# Nobuhisa Hagiwara, MD,** Dominic J. Allocco, MD,†† Keith D. Dawkins, MD,†† for the PLATINUM Trial Investigators

*New York, New York; La Jolla, California; Clayton, Victoria, Australia; Toulouse, France;
Leuven and Genk, Belgium; Ocala, Florida; Tokyo, Japan; and Natick, Massachusetts*

Stone GW et al. J Am Coll Cardiol 2011;57:1700-8.